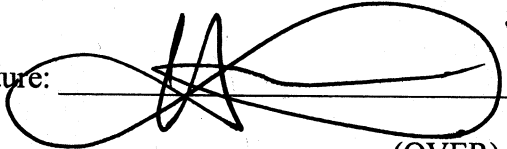


VERIFICATION OF CALIBRATION REPORT MAY 04 2009

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N: <u>130298</u> ✓
Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>1 May 09</u> ✓		
A	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>	
	Instrument Location: <u>Palmer Police Department</u>	
Alco S/N: <u>X124627</u> ✓ Target Value: <u>.084</u> ✓ High Pressure: <u>1350</u>		
B	Alco Test Value Average: <u>.084</u> ✓ 1 st Alco	<u>.084</u> ✓ 2 nd Alco
Signature: 		<u>CUB</u> <u>5/8/09</u>
(OVER)		

I, Nita J. Bolz, after being first duly sworn, depose and state as follows below) (Do Not write in following)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program


Subscribed and sworn before me this 22 day of May 2009.

 (Notary Seal Stamp)

Carolyn M. Noland

Notary Public, State of Alaska

Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

~~01-01-2009~~ ✓ *SPB 5/16/09*
OPERATOR'S NAME:
GIPSON/JAMES/C
OPERATOR'S NUMBER: 4842
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
RJCSO
O.L. #: 0123456
DEPT/AGENCY: PLM1
CASE/REPORT: 01-2345
TEST TYPE: V ✓
ALCO TARGET VALUE: .084 ✓
~~ALCO C-10-1004007~~

— BREATH ANALYSIS —

.084 ADJUSTED FOR 30.22 in
ALCO TARGET .084 07:59
BLANK TEST .000 08:00
INTERNAL STANDARD VERIFIED 08:00
ALCO TV 30.22 in .084 ✓ 08:01
BLANK TEST .000 08:01
SUBJECT SAMPLE .000 08:02
BLANK TEST .000 ✓ 08:03
ALCO TV 30.22 in .084 ✓ 08:03
BLANK TEST .000 08:04

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

MAY 01, 2009 ✓
TIME 07:57

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATHER TUBE: 42c
BAROMETER: 30.22 in
FLOW DETECTOR: OKAY
PUMP
PUMP SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~